



Performance Verification Manual

DP800 Series Programmable Linear DC Power Supply

**Jun. 2016
RIGOL Technologies, Inc.**

Guaranty and Declaration

Copyright

© 2014 RIGOL Technologies, Inc. All Rights Reserved.

Trademark Information

RIGOL is a registered trademark of RIGOL Technologies, Inc.

Publication Number

PVH03101-1110

Notices

- **RIGOL** products are covered by P.R.C. and foreign patents, issued and pending.
- **RIGOL** reserves the right to modify or change parts of or all the specifications and pricing policies at the company's sole decision.
- Information in this publication replaces all previously released materials.
- Information in this publication is subject to change without notice.
- **RIGOL** shall not be liable for either incidental or consequential losses in connection with the furnishing, use, or performance of this manual, as well as any information contained.
- Any part of this document is forbidden to be copied, photocopied, or rearranged without prior written approval of **RIGOL**.

Product Certification

RIGOL guarantees this product conforms to the national and industrial standards in China as well as the ISO9001:2008 standard and the ISO14001:2004 standard. Other international standard conformance certification is in progress.

Contact Us

If you have any problem or requirement when using our products or this manual, please contact **RIGOL**.

E-mail: service@rigol.com

Website: www.rigol.com

General Safety Summary

Please review the following safety precautions carefully before putting the instrument into operation so as to avoid any personal injury or damage to the instrument and any product connected to it. To prevent potential hazards, please follow the instructions specified in this manual to use the instrument properly.

Use Proper Power Cord.

Only the exclusive power cord designed for the instrument and authorized for use within the local country could be used.

Ground the Instrument.

The instrument is grounded through the Protective Earth lead of the power cord. To avoid electric shock, connect the earth terminal of the power cord to the Protective Earth terminal before connecting any input or output terminals.

Connect the Probe Correctly.

If a probe is used, the probe ground lead must be connected to earth ground. Do not connect the ground lead to high voltage. Improper way of connection could result in dangerous voltages being present on the connectors, controls or other surfaces of the oscilloscope and probes, which will cause potential hazards for operators.

Observe All Terminal Ratings.

To avoid fire or shock hazard, observe all ratings and markers on the instrument and check your manual for more information about ratings before connecting the instrument.

Use Proper Overvoltage Protection.

Ensure that no overvoltage (such as that caused by a bolt of lightning) can reach the product. Otherwise, the operator might be exposed to the danger of an electric shock.

Do Not Operate Without Covers.

Do not operate the instrument with covers or panels removed.

Do Not Insert Objects Into the Air Outlet.

Do not insert objects into the air outlet, as doing so may cause damage to the instrument.

Use Proper Fuse.

Please use the specified fuses.

Avoid Circuit or Wire Exposure.

Do not touch exposed junctions and components when the unit is powered on.

Do Not Operate With Suspected Failures.

If you suspect that any damage may occur to the instrument, have it inspected by **RIGOL** authorized personnel before further operations. Any maintenance, adjustment or replacement especially to circuits or accessories must be performed by **RIGOL** authorized personnel.

Provide Adequate Ventilation.

Inadequate ventilation may cause an increase of temperature in the instrument, which would cause damage to the instrument. So please keep the instrument well ventilated and inspect the air outlet and the fan regularly.

Do Not Operate in Wet Conditions.

To avoid short circuit inside the instrument or electric shock, never operate the instrument in a humid environment.

Do Not Operate in an Explosive Atmosphere.

To avoid personal injuries or damage to the instrument, never operate the instrument in an explosive atmosphere.

Keep Instrument Surfaces Clean and Dry.

To avoid dust or moisture from affecting the performance of the instrument, keep the surfaces of the instrument clean and dry.

Prevent Electrostatic Impact.

Operate the instrument in an electrostatic discharge protective environment to avoid damage induced by static discharges. Always ground both the internal and external conductors of cables to release static before making connections.

Use the Battery Properly.

Do not expose the battery (if available) to high temperature or fire. Keep it out of the reach of children. Improper change of a battery (lithium battery) may cause an explosion. Use the **RIGOL** specified battery only.

Handle with Caution.

Please handle with care during transportation to avoid damage to keys, knobs, interfaces, and other parts on the panels.

Allgemeine Sicherheits Informationen

Überprüfen Sie die folgenden Sicherheitshinweise sorgfältig um Personenschäden oder Schäden am Gerät und an damit verbundenen weiteren Geräten zu vermeiden. Zur Vermeidung von Gefahren, nutzen Sie bitte das Gerät nur so, wie in diesem Handbuch angegeben.

Um Feuer oder Verletzungen zu vermeiden, verwenden Sie ein ordnungsgemäßes Netzkabel.

Verwenden Sie für dieses Gerät nur das für ihr Land zugelassene und genehmigte Netzkabel.

Erden des Gerätes.

Das Gerät ist durch den Schutzleiter im Netzkabel geerdet. Um Gefahren durch elektrischen Schlag zu vermeiden, ist es unerlässlich, die Erdung durchzuführen. Erst dann dürfen weitere Ein- oder Ausgänge verbunden werden.

Anschluss eines Tastkopfes.

Die Erdungsklemmen der Sonden sind auf dem gleichen Spannungspegel des Instruments geerdet. Schließen Sie die Erdungsklemmen an keine hohe Spannung an.

Beachten Sie alle Anschlüsse.

Zur Vermeidung von Feuer oder Stromschlag, beachten Sie alle Bemerkungen und Markierungen auf dem Instrument. Befolgen Sie die Bedienungsanleitung für weitere Informationen, bevor Sie weitere Anschlüsse an das Instrument legen.

Verwenden Sie einen geeigneten Überspannungsschutz.

Stellen Sie sicher, daß keinerlei Überspannung (wie z.B. durch Gewitter verursacht) das Gerät erreichen kann. Andernfalls besteht für den Anwender die Gefahr eines Stromschlages.

Nicht ohne Abdeckung einschalten.

Betreiben Sie das Gerät nicht mit entfernten Gehäuse-Abdeckungen.

Betreiben Sie das Gerät nicht geöffnet.

Der Betrieb mit offenen oder entfernten Gehäuseteilen ist nicht zulässig. Nichts in entsprechende Öffnungen stecken (Lüfter z.B.)

Passende Sicherung verwenden.

Setzen Sie nur die spezifikationsgemäßen Sicherungen ein.

Vermeiden Sie ungeschützte Verbindungen.

Berühren Sie keine unisolierten Verbindungen oder Baugruppen, während das Gerät in Betrieb ist.

Betreiben Sie das Gerät nicht im Fehlerfall.

Wenn Sie am Gerät einen Defekt vermuten, sorgen Sie dafür, bevor Sie das Gerät wieder betreiben, dass eine Untersuchung durch qualifiziertes Kundendienstpersonal durchgeführt wird. Jedwede Wartung, Einstellarbeiten oder Austausch von Teilen am Gerät, sowie am Zubehör dürfen nur von **RIGOL** autorisiertem Personal durchgeführt werden.

Belüftung sicherstellen.

Unzureichende Belüftung kann zu Temperaturanstiegen und somit zu thermischen Schäden am Gerät führen. Stellen Sie deswegen die Belüftung sicher und kontrollieren regelmäßig Lüfter und Belüftungsöffnungen.

Nicht in feuchter Umgebung betreiben.

Zur Vermeidung von Kurzschluß im Geräteinneren und Stromschlag betreiben Sie das Gerät bitte niemals in feuchter Umgebung.

Nicht in explosiver Atmosphäre betreiben.

Zur Vermeidung von Personen- und Sachschäden ist es unumgänglich, das Gerät ausschließlich fernab jedweder explosiven Atmosphäre zu betreiben.

Geräteoberflächen sauber und trocken halten.

Um den Einfluß von Staub und Feuchtigkeit aus der Luft auszuschließen, halten Sie bitte die Geräteoberflächen sauber und trocken.

Schutz gegen elektrostatische Entladung (ESD).

Sorgen Sie für eine elektrostatisch geschützte Umgebung, um somit Schäden und Funktionsstörungen durch ESD zu vermeiden. Erden Sie vor dem Anschluß immer Innen- und Außenleiter der Verbindungsleitung, um statische Aufladung zu entladen.

Die richtige Verwendung des Akku.

Wenn eine Batterie verwendet wird, vermeiden Sie hohe Temperaturen bzw. Feuer ausgesetzt werden. Bewahren Sie es außerhalb der Reichweite von Kindern auf. Unsachgemäße Änderung der Batterie (Anmerkung: Lithium-Batterie) kann zu einer Explosion führen. Verwenden Sie nur von RIGOL angegebene Akkus.

Sicherer Transport.

Transportieren Sie das Gerät sorgfältig (Verpackung!), um Schäden an Bedienelementen, Anschlüssen und anderen Teilen zu vermeiden.

Vermeiden Sie das Einprägen von Strom und Spannung an den Testklemmen.

Das DP800 Power Supply kann hierdurch zerstört werden, keine aktive Last. Das DP800 kann nur Strom und Spannungen liefern.

Document Overview

DP800 series is a high-performance programmable DC power supply. This manual introduces the performance verification test methods of DP800 series. The performance verification test mainly verifies whether DP800 series programmable linear DC power supply can work normally and is within specifications.

Main topics of this manual

Chapter 1 Test Overview

This chapter introduces the test preparations, the recommended test devices, the test precautions as well as the test result record and so on.

Chapter 2 Constant Voltage Tests

This chapter introduces the specification test methods of DP800 under constant voltage (CV) mode.

Chapter 3 Constant Current Tests

This chapter introduces the specification test methods of DP800 under constant current (CC) mode.

Appendix

Provide the test result record forms and the performance specifications of all models of DP800 series programmable linear DC power supply.

Content Conventions in this Manual

DP800 series programmable linear DC power supply includes the following models. Unless specified otherwise in this manual, DP831A is taken as an example to illustrate the performance verification test methods of DP800 series.

Model	Channel	Output Voltage/Current
DP831A/DP831	3	8V/5A, 30V/2A, -30V/2A
DP832A/DP832	3	30V/3A, 30V/3A, 5V/3A
DP821A/DP821	2	60V/1A, 8V/10A
DP811A/DP811	1	20V/10A (Range 1), 40V/5A (Range 2)

Contents

Guaranty and Declaration	I
General Safety Summary	II
Allgemeine Sicherheits Informationen.....	IV
Document Overview.....	VI
Chapter 1 Test Overview	1-1
Test Preparations.....	1-2
Voltage and Current Values	1-4
Recommended Test Devices	1-5
Test Precautions.....	1-6
Test Result Record.....	1-6
Chapter 2 Constant Voltage Tests	2-1
Preparations	2-2
CV Load Regulation Rate (CV Load Effect)	2-4
CV Linear Regulation Rate (CV Source Effect).....	2-8
CV Ripple and Noise	2-13
Transient Response Time	2-18
CV Programming and Readback Accuracy	2-23
Chapter 3 Constant Current Tests.....	3-1
Preparations	3-2
CC Load Regulation Rate (CC Load Effect)	3-4
CC Linear Regulation Rate (CC Source Effect).....	3-8
CC Ripple and Noise (Normal Mode).....	3-13
CC Programming and Readback Accuracy	3-17
Appendix.....	1
Appendix A: Test Result Record Forms.....	1
DP831A Performance Verification Test Record Form.....	1
DP831 Performance Verification Test Record Form	5
DP832A Performance Verification Test Record Form.....	9
DP832 Performance Verification Test Record Form	13
DP821A Performance Verification Test Record Form.....	17
DP821 Performance Verification Test Record Form	21
DP811A Performance Verification Test Record Form.....	25
DP811 Performance Verification Test Record Form	29
Appendix B: Specifications	33
DP832A/DP831A/DP821A/DP811A Specifications	33
DP831/DP832/DP821/DP811 Specifications	37

Chapter 1 Test Overview

Topics of this chapter:

- Test Preparations
- Voltage and Current Values
- Recommended Test Devices
- Test Precautions
- Test Result Record

Test Preparations

You need to finish the following preparations before performing the performance verification test.

1. Perform self-test to make sure that the instrument can work normally.

Connect the instrument to AC power supply using the power cord provided with the accessories. Press the power switch key at the front panel; the instrument starts and performs self-test. You can press **Utility** → **Test/Cal** after power-on to examine the self-test information (including the top board, bottom board, fan and temperature). If the self-test fails, please turn off and then turn on the instrument to perform the self-test again and examine the self-test information. If the self-test still fails, please contact **RIGOL**. Make sure that the reason that results in the self-test failure are found and solved. Perform the performance verification test only after the instrument passes the self-test.

Notes:

- Before connecting the power, make sure that the setting of the voltage selector at the rear panel of the power supply matches the AC power supply to be connected and the fuse currently installed matches the input voltage. The input voltages supported by DP800 series and the matching fuses are as shown in the table below.

DP831A/DP831/DP821A/DP821	
100	100Vac ± 10%, 50Hz to 60Hz, T5A fuse
115	115Vac ± 10%, 50Hz to 60Hz, T5A fuse
230	230Vac ± 10% (maximum 250Vac), 50Hz to 60Hz, T2.5A fuse
DP832A/DP832/DP811A/DP811	
100	100Vac ± 10%, 50Hz to 60Hz, T6.3A fuse
115	115Vac ± 10%, 50Hz to 60Hz, T6.3A fuse
230	230Vac ± 10% (maximum 250Vac), 50Hz to 60Hz, T3.15A fuse

Note: The upper limit of the input voltage supported by DP800 series is 250Vac.

- Before performing the self-test, make sure that there is no connection at the front and rear panel terminals of the power supply.
2. Make sure that the power supply is within the calibration period (1 year). If calibration is required, please contact **RIGOL**.
 3. Run the instrument for at least 30 minutes.
 4. Make sure that the environment temperature is between 20°C and 30°C and the relative humidity is less than 80%.

5. The test connecting wires used should be as short as possible. For the channels that support the Sense function (DP811A/DP811 and CH2 of DP821A/DP821), please short-circuit the (S+) and (+) terminals, (S-) and (-) terminals (as shown in Figure 2-2 or Figure 3-2) of the channels respectively and turn on the Sense function of the corresponding channel before performing the test.

Note:

The tests introduced in this manual should be performed by professionals. During the tests, there might be dangerous voltage at the output terminals of the power supply as well as certain test devices.

Voltage and Current Values

During the test, you need to set the voltage and current of the output channels (output ranges) of the power supply to specified values. The rated output values and maximum output values of the voltage and current of each channel of various models of DP800 series are listed in Table 1-1.

Table 1-1 Voltage and Current Values of the Channels (Ranges) of DP800 Series

Channel (Range)	Rated Output Voltage	Max Output Voltage	Rated Output Current	Max Output Current
DP831A/DP831				
CH1	8V	8.4V	5A	5.3A
CH2	30V	32V	2A	2.1A
CH3	-30V	-32V	2A	2.1A
DP832A/DP832				
CH1	30V	32V	3A	3.2A
CH2	30V	32V	3A	3.2A
CH3	5V	5.3V	3A	3.2A
DP821A/DP821				
CH1	60V	63V	1A	1.05A
CH2	8V	8.4V	10A	10.5A
DP811A/DP811				
Range1	20V	21V	10A	10.5A
Range2	40V	42V	5A	5.3A

Recommended Test Devices

It is recommended that you use the test devices listed in the table below or other test devices whose performance specifications satisfy the "Performance Requirement" listed in the table below to test the performance specifications of the DP800 series.

Table 1-2 Recommended Test Devices

Device	Performance Requirement	Recommended Instrument	Use
Digital Oscilloscope	Bandwidth: $\geq 20\text{MHz}$ Minimum Vertical Scale: $\leq 2\text{mV/div}$ Bandwidth Limit: $\leq 20\text{MHz}$	RIGOL DS1102E	Measure ripple and noise, transient response time
Digital Multimeter	Readout Resolution: $6\frac{1}{2}$	RIGOL DM3068	Measure dc voltage
RMS Voltmeter	Sensitivity: 1mV Bandwidth: $\geq 10\text{MHz}$		Measure rms ripple and noise
Electronic Load	Voltage Range: 80Vdc Current Range: 60A dc Maximum Power: 300W Dynamic frequency: 1kHz	Chroma 63103A	Measure load regulation rate, linear regulation rate, transient response time
AC Power Supply	Regulation Rate: $>1\%$	Chroma 61602	—
Resistive Load R_L	0.8Ω (200W) 1.6Ω (100W) 2Ω (400W) 8Ω (400W) 10Ω (200W) 15Ω (200W) 60Ω (200W)	—	Measure ripple and noise
Current Sampling Resistor R_M	0.022Ω (5W , temperature drift: 10ppm)	—	Measure load regulation rate, linear regulation rate, programming accuracy and readback accuracy
Multimeter Test Probe	—	—	—
USB Cable	USB Device to USB Host, for connecting the power supply and PC	—	—
Short Circuit Device (2)	—	—	Short-circuit the (S+) and (+) terminals, (S-) and (-) terminals of the channel that supports the Sense function

Test Precautions

The output terminal of the power supply is as shown in Figure 1-1. The output terminal is a metal conductor with certain contact resistance (Δr) and when the output current of the power supply is I , the voltage of this terminal is $V_e = \Delta r \times I$. Therefore, during the test process, the voltage test point is always located at A to reduce the error caused by the terminal voltage as far as possible. Besides, the contact resistance between this terminal and the power output wire/the voltage feedback wire inside the instrument chassis can also cause error (about 2mV, called U_{offset}).

When testing the load regulation rate, voltage peak-peak value and transient response time, the test devices are connected to the output terminal via A and the load resistor is connected to the output terminal via B.

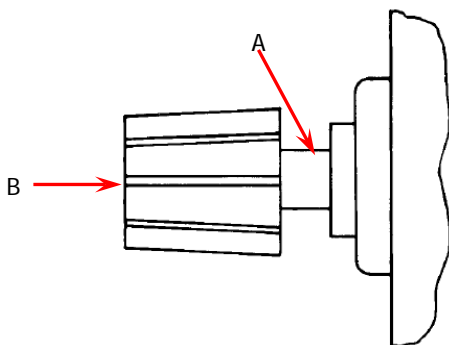


Figure 1-1 Output Terminal

During the test, please pay attention to shield the effect of the environmental space radiation noise on the test effectively.

Test Result Record

Record and keep the test results of each test item. The test result record forms, which provide all the test items and the corresponding performance specification limits as well as spaces for users to record the test results, of all models of DP800 series programmable linear DC power supply are provided in “**Appendix A: Test Result Record Forms**” of this manual.

Tip:

It is recommended that you photocopy the desired test result record form before each test. During the test process, record the test results on the copies so that the forms can be used repeatedly.

Chapter 2 Constant Voltage Tests

Topics of this chapter:

- Preparations
- CV Load Regulation Rate (CV Load Effect)
- CV Linear Regulation Rate (CV Source Effect)
- CV Ripple and Noise
- Transient Response Time
- CV Programming and Readback Accuracy

Preparations

When the power supply is in CV state, the main parameters to be tested include CV load regulation rate, CV linear regulation rate, CV ripple and noise, transient response time, CV programming and readback accuracy.

Before performing the tests, select the appropriate voltage via the “voltage selector” at the rear panel of the power supply according to the AC line voltage of the country (230V is taken as an example in all the tests in this manual). Under normal temperature (about 25°C), make connections according to Figure 2-1 or Figure 2-2 using the devices recommended in **“Recommended Test Devices”**. During the test process, please set the voltage of the AC power supply according to the voltage selected of the “voltage selector” at the rear panel of the power supply.

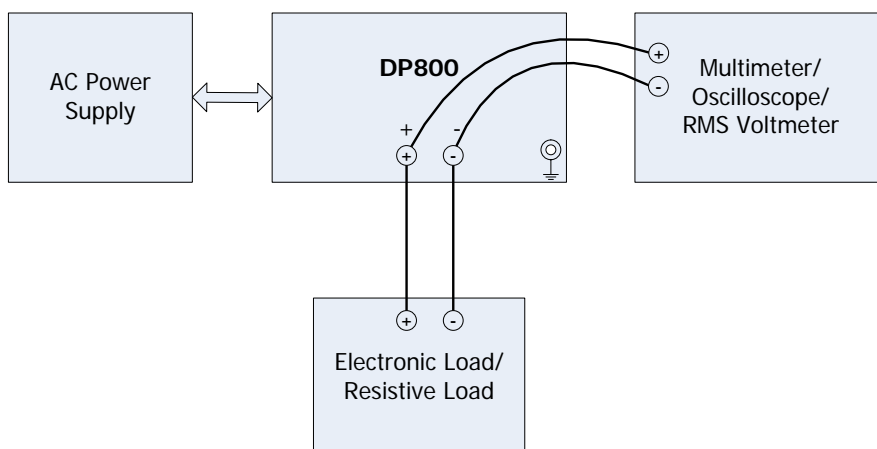


Figure 2-1 CV Test Connections

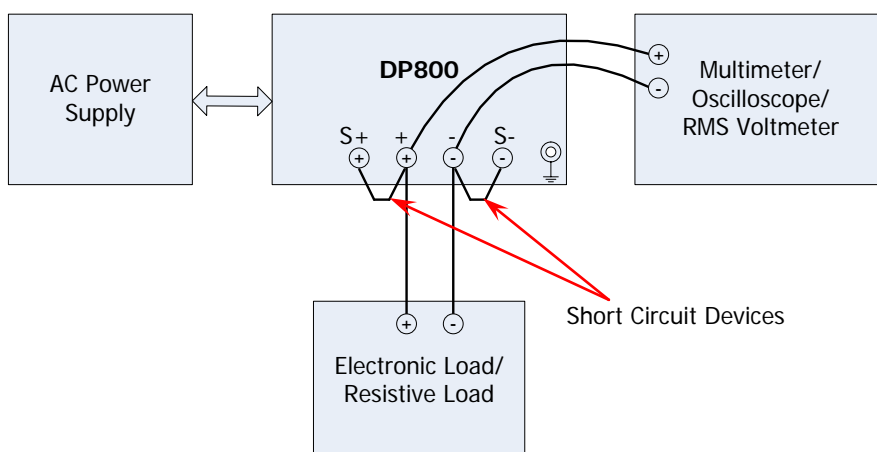


Figure 2-2 CV Test Connections (Sense)

Note: During the CV tests, make connections according to Figure 2-1 for the normal channels (namely the channels that do not support the Sense function) of the DP800 series power supply. For the channels that support the Sense function (DP811A/DP811 and CH2 of DP821A/DP821) make connections according to Figure 2-2 (note to short-circuit the (S+) and (+) terminals, (S-) and (-) terminals of the channel respectively) and turn on the Sense function of the channel during the test process to measure the specifications under Sense mode.

CV Load Regulation Rate (CV Load Effect)

CV load regulation rate refers to the relation between the variation of the output voltage (caused by the load effect) and the rated output voltage when the power supply is under CV output mode.

DP831A is taken as an example to test the CV load regulation rate of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Load Regulation Rate, \pm (Output Percentage+Offset)	
Voltage	<0.01%+2mV

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, electronic load and multimeter according to Figure 2-1. Both the electronic load and multimeter are connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.
2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 2-1. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.
4. Turn on the electronic load. Adjust the current of the electronic load to 0A or do not connect any load device (no load).
5. Turn on the digital multimeter; select DC voltage measurement function and set the range to “Auto”. Make sure that the power supply is in CV mode. Read and record the reading (U_0) of the multimeter.
6. Set the electronic load to work in CC mode and adjust the current of the electronic load to the rated output current (please refer to Table 1-1) of the

channel (range) under test. Make sure that the power supply is in CV mode. Read and record the reading (U_1) of the multimeter.

7. Calculate the voltage variation (namely the CV load effect, $|U_1 - U_0|$) and compare it with the specified specification in Table 2-1.
8. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
9. Repeat steps 1 to 8 to test the CV load regulation rates of CH2 and CH3 until finishing the CV load regulation rate tests of all channels.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform steps 4 to 8 to test the CV load regulation rate of this range. Then, repeat steps 3 to 8 to test the CV load regulation rate of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, electronic load and multimeter according to Figure 2-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 2-1 DP831A CV Load Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

Table 2-2 DP831 CV Load Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

Table 2-3 DP832A CV Load Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

Table 2-4 DP832 CV Load Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

Table 2-5 DP821A CV Load Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

Table 2-6 DP821 CV Load Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

Table 2-7 DP811A CV Load Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

Table 2-8 DP811 CV Load Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

CV Linear Regulation Rate (CV Source Effect)

CV linear regulation rate refers to the relation between the variation of the output voltage (caused by the variation of the input power) and the rated output voltage when the power supply is under CV output mode.

DP831A is taken as an example to test the CV linear regulation rate of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Linear Regulation Rate, \pm (Output Percentage+Offset)	
Voltage	<0.01%+2mV

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, electronic load and multimeter according to Figure 2-1. Both the electronic load and multimeter are connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.

Note: Set the voltage selector (100, 115 or 230) at the rear panel of DP800 according to your need and make sure that the fuse currently installed matches the actual input voltage (please refer to Table 2-9). As the test methods when selecting different voltages are the same, 230V is taken as an example for illustration.

2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 2-10. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.
4. Turn on the electronic load; set the electronic load to work in CC mode and adjust the current of the electronic load to the rated output current (please refer to Table 1-1) of the channel (range) under test.

5. Turn on the digital multimeter; select DC voltage measurement function and set the range to "Auto". Make sure that the power supply is in CV mode. Read and record the reading (U_0) of the multimeter.
6. Adjust the AC power supply to undervoltage state (namely the amplitude reduces by 10%, refer to Table 2-9); read and record the reading (U_1) of the multimeter. Adjust the AC power supply to overvoltage state (namely the amplitude increases by 10%, refer to Table 2-9); read and record the reading (U_2) of the multimeter.
Note: The upper limit of the overvoltage of DP800 series is 250Vac.
7. Calculate the voltage variations (namely the CV source effect, $|U_1-U_0|$ and $|U_2-U_0|$) and compare them with the specified specifications in Table 2-10.
8. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
9. Repeat steps 1 to 8 to test the CV linear regulation rates of CH2 and CH3 until finishing the CV linear regulation rate tests of all channels.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform step 4 to step 8 to test the CV linear regulation rate of this range. Then, repeat step 3 to step 8 to test the CV linear regulation rate of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, electronic load and multimeter according to Figure 2-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Table 2-9 AC Power Supply Setting Form

DP831A/DP831/DP821A/DP821			
Voltage Selector	100	115	230
Fuse	T5A	T5A	T2.5A
Undervoltage (Vac)	90	103	207
Overvoltage (Vac)	110	127	250
DP832A/DP832/DP811A/DP811			
Voltage Selector	100	115	230
Fuse	T6.3A	T6.3A	T3.15A
Undervoltage (Vac)	90	103	207
Overvoltage (Vac)	110	127	250

Test Record Forms:

Table 2-10 DP831A CV Linear Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 $			
	$ U_2-U_0 $			

Table 2-11 DP831 CV Linear Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 $			
	$ U_2-U_0 $			

Table 2-12 DP832A CV Linear Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 $			
	$ U_2-U_0 $			

Table 2-13 DP832 CV Linear Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 $			
	$ U_2 - U_0 $			

Table 2-14 DP821A CV Linear Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 $		
	$ U_2 - U_0 $		

Table 2-15 DP821 CV Linear Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 $		
	$ U_2 - U_0 $		

Table 2-16 DP811A CV Linear Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 $		
	$ U_2-U_0 $		

Table 2-17 DP811 CV Linear Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 $		
	$ U_2-U_0 $		

CV Ripple and Noise

When the power supply is working in CV mode, the combination of the periodic and random deviations (PARD) when outputting DC voltage is equivalent to superimposing a residual AC voltage on the DC output voltage. This residual AC voltage, namely the ripple and noise (usually, ripple is periodic offset while noise is random offset), can be expressed in RMS or peak-to-peak value form.

DP831A is taken as an example to test the CV ripple and noise of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set and select the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Ripple and Noise (20Hz-20MHz)	
Normal Mode Voltage	DP831A/DP831/DP832A/DP832/DP821A/DP821: <350 μ Vrms/2mVpp DP811A/DP811: <350 μ Vrms/3mVpp

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, resistive load and oscilloscope according to Figure 2-1. Both the resistive load and oscilloscope are connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.

Notes:

- Do not connect the negative terminal of the output terminal of the channel to be tested to the shielding ground; otherwise, a ground loop would be formed. In Figure 2-3, the connection in figure A forms a ground loop while figure B shows the correct connection.

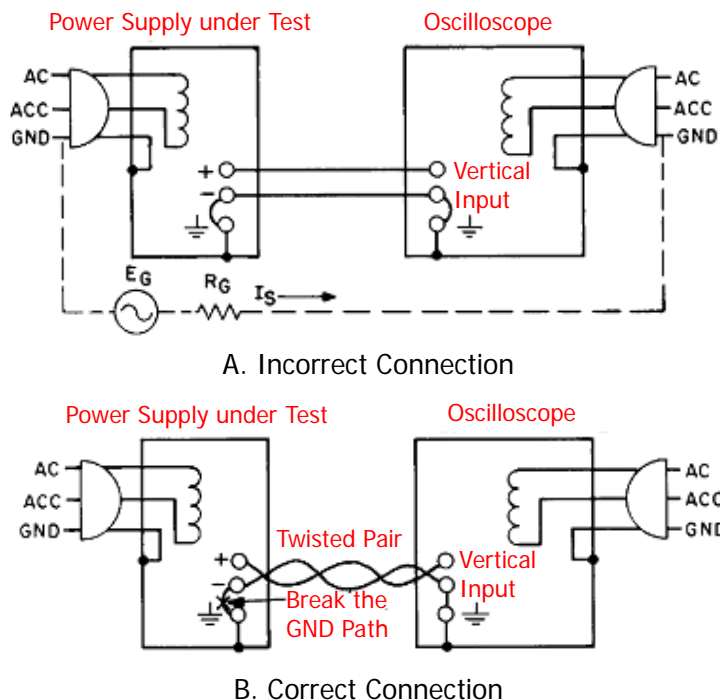


Figure 2-3 Peak-peak Value Measurement Connections

- Please use resistive load instead of electronic load to avoid the effect on the noise measurement of the power supply caused by the electronic load noise. Please refer to Table 2-18 for the resistance of the resistive load.
 - Connect the positive terminal of the oscilloscope probe to the positive terminal (+) of the output terminals of the channel under test of the power supply and connect the ground terminal of the oscilloscope probe to the negative terminal (-) of the output terminals of the channel under test of the power supply. During the test, please ensure the effective contact. Note that you are recommended to use ground spring as ground wire so as to minimize the current coupling area between the probe tip and the ground wire and to minimize the space radiation interference.
2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 2-18. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.

4. Turn on the oscilloscope and set the oscilloscope parameters. Set the timebase to 5ms/div, the vertical scale to 2mV, the sample mode to peak detect, the coupling mode to AC and the trigger source to AC Line. The input impedance is 1M Ω . Enable the 20MHz bandwidth limit and then enable the peak-peak value measurement function of the oscilloscope. Make sure that the power supply is in CV mode. Read and record the peak-peak value (V_{pp}) measured by the oscilloscope and compare it with the specified specification in Table 2-18.
 5. Turn off the oscilloscope and disconnect the connection between DP800 and the oscilloscope. Connect DP800, AC power supply, resistive load and RMS voltmeter according to Figure 2-1. Turn on the RMS voltmeter and select the AC voltage random measurement mode (SETACV RNDM). Make sure that the power supply is in CV mode. Read and record the RMS value (V_{rms}) measured by the RMS voltmeter and compare it with the specified specification in Table 2-18.
- Note:** The measurement wires of the RMS voltmeter should be twisted together to minimize the effect of the space radiation noise on the test as much as possible.
6. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
 7. Repeat steps 1 to 6 to test the CV ripple and noise of CH2 and CH3 until finishing the CV ripple and noise tests of all channels.

Notes:

- During the CV ripple and noise test, please pay attention to shield the effect of the environmental space radiation noise on the test effectively.
- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform step 4 to step 6 to test the CV ripple and noise of this range. Then, repeat step 3 to step 6 to test the CV ripple and noise of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, resistive load and oscilloscope (RMS voltmeter) according to Figure 2-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 2-18 DP831A CV Ripple and Noise Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<350 μ Vrms/2mVpp		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Table 2-19 DP831 CV Ripple and Noise Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<350 μ Vrms/2mVpp		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Table 2-20 DP832A CV Ripple and Noise Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<350 μ Vrms/2mVpp		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Table 2-21 DP832 CV Ripple and Noise Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<350 μ Vrms/2mVpp		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Table 2-22 DP821A CV Ripple and Noise Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ Vrms/2mVpp	
Resistive Load R_L		60 Ω	0.8 Ω
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Table 2-23 DP821 CV Ripple and Noise Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ Vrms/2mVpp	
Resistive Load R_L		60 Ω	0.8 Ω
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Table 2-24 DP811A CV Ripple and Noise Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<350 μ Vrms/3mVpp	
Resistive Load R_L		2 Ω	8 Ω
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Table 2-25 DP811A CV Ripple and Noise Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<350 μ Vrms/3mVpp	
Resistive Load R_L		2 Ω	8 Ω
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Transient Response Time

Transient response time refers to the time required for the output voltage of the power supply to recover to within 15mV following a transient variation in the load current (50% transient variation, namely the output current changes from full load to half load or vice versa). As shown in Figure 2-4, t is the transient response time.

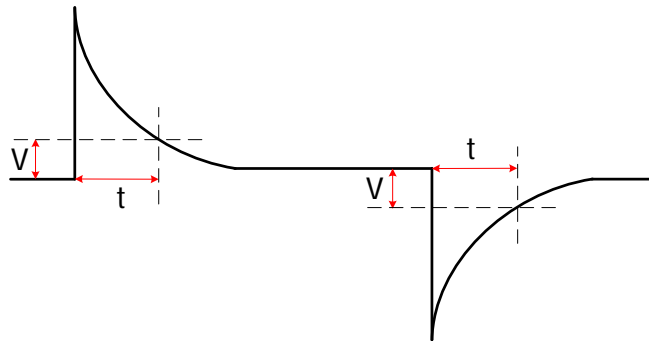


Figure 2-4 Transient Response Time

DP831A is taken as an example to test the transient response time of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:


Transient Response Time
Less than 50 μ s for output voltage to recover to within 15 mV following a change in output current from full load to half load or vice versa.

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, electronic load and oscilloscope according to Figure 2-1. Both the electronic load and oscilloscope are connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3
2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 2-26. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.
4. Turn on the electronic load and set the electronic load parameters. Select the CC dynamic response mode (CCDH mode); set CCDH1 to the rated current value of the channel (range) under test, CCDH2 to the current value of the channel (range) under test with half load (for the CCDH1 and CCDH2 values, please refer to Table 2-26), CCDHT1 and CCDHT2 to 500 μ s (namely 1kHz frequency and 50% duty cycle), the rising edge time and falling edge time to 250mA/ μ s. Turn on the electronic load and make sure that the programmable electronic load is in CC mode.
5. Turn on the oscilloscope and set the oscilloscope parameters. Set the coupling mode to AC, the trigger source to AC Line and enable the 20MHz bandwidth limit. Enable the cursor measurement function and measure the transient response time (namely ΔX) displayed on the screen of the oscilloscope, as shown in the figure below, and compare it with the specified specification in Table 2-26.

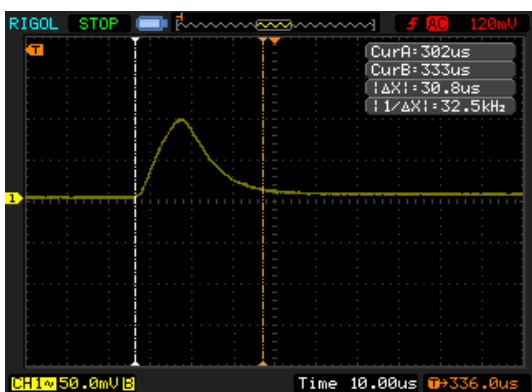

6. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
7. Repeat steps 1 to 6 to test the transient response time of CH2 and CH3 until finishing the transient response time tests of all channels.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform step 4 to step 6 to test the transient response time of this range. Then, repeat step 3 to step 6 to test the transient response time of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, electronic load and oscilloscope according to Figure 2-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 2-26 DP831A Transient Response Time Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<50 μ s		
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Electronic Load Current Setting	CCDH1	5A	2A	2A
	CCDH2	2.5A	1A	1A
Measurement Result	t			

Table 2-27 DP831 Transient Response Time Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<50 μ s		
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Electronic Load Current Setting	CCDH1	5A	2A	2A
	CCDH2	2.5A	1A	1A
Measurement Result	t			

Table 2-28 DP832A Transient Response Time Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<50μs		
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Electronic Load Current Setting	CCDH1	3A	3A	3A
	CCDH2	1.5A	1.5A	1.5A
Measurement Result	t			

Table 2-29 DP832 Transient Response Time Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<50μs		
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Electronic Load Current Setting	CCDH1	3A	3A	3A
	CCDH2	1.5A	1.5A	1.5A
Measurement Result	t			

Table 2-30 DP821A Transient Response Time Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<50μs	
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Electronic Load Current Setting	CCDH1	1A	10A
	CCDH2	0.5A	5A
Measurement Result	t		

Table 2-31 DP821 Transient Response Time Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<50μs	
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Electronic Load Current Setting	CCDH1	1A	10A
	CCDH2	0.5A	5A
Measurement Result	t		

Table 2-32 DP811A Transient Response Time Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<50μs	
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Electronic Load Current Setting	CCDH1	10A	5A
	CCDH2	5A	2.5A
Measurement Result	t		

Table 2-33 DP811 Transient Response Time Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<50μs	
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Electronic Load Current Setting	CCDH1	10A	5A
	CCDH2	5A	2.5A
Measurement Result	t		

CV Programming and Readback Accuracy

CV programming accuracy refers to the error between the voltage setting of the channel and the actual output voltage value when the power supply is in CV mode; CV readback accuracy refers to the error between the actual output voltage value and the readback voltage value when the power supply is in CV mode.

DP831A is taken as an example to test the CV programming and readback accuracy of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Annual Accuracy ^[1] (25℃±5℃)± (Output Percentage+Offset)			
Channel		Programming	Readback
DP831A/DP831	CH1	0.1%+5mV	0.1%+5mV
	CH2	0.05%+20mV	0.05%+10mV
	CH3	0.05%+20mV	0.05%+10mV
DP832A/DP832	CH1	0.05%+20mV	0.05%+10mV
	CH2	0.05%+20mV	0.05%+10mV
	CH3	0.1%+5mV	0.1%+5mV
DP821A/DP821	CH1	0.1%+25mV	0.1%+25mV
	CH2	0.05%+10mV	0.05%+5mV
DP811A/DP811	CH1	0.05%+10mV	0.05%+10mV

Note^[1]: The accuracy parameters are acquired via calibration under 25℃ after 1-hour warm-up.

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply and multimeter according to Figure 2-1. The multimeter is connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3. Then, connect the power supply with PC (take the connection via USB cable as an example) via the remote interfaces (USB, GPIB, LAN).
2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Measure the CV programming and readback accuracy (take CH1 as an example

in this place) when the output voltage is 0V.

- 1) Turn on DP800. Send the following commands via the remote interface to select the channel to be tested (namely the current channel), set the voltage and current of this channel (please refer to Table 2-34) as well as enable the output of this channel.

```
:APPL CH1,0,5.3      /*Select CH1 as the current channel and set the
                        voltage and current of this channel to 0V and
                        5.3A respectively*/
```

```
:OUTP CH1,ON         /*Enable the output of CH1*/
```

Notes:

- The above commands are only applicable to the multi-channel models of DP800. You can also send the `:INST:NSEL 1` (or `:INST CH1`) command to select CH1 as the current channel, the `:SOUR1:VOLT 0` command to set the voltage of CH1 to 0V and the `:SOUR1:CURREN 5.3` command to set the current of CH1 to 5.3A.
- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), you can send the `:OUTP:RANG P20V` (or `:OUTP:RANG LOW`, or `:VOLT:RANG P20V`, or `:VOLT:RANG LOW`) command to select Range1 as the current range and then send the `:VOLT 0` command to set the voltage of the channel to 0V and the `:CURREN 10.5` command to set the current of the channel to 10.5A.

- 2) Turn on the digital multimeter; select DC voltage measurement function and set the range to "Auto". Make sure that the power supply is in CV mode. Read and record the reading (U_1) of the multimeter.
- 3) Send the `:MEAS:VOLT? CH1` command via the remote interface; read and record the returned voltage value U_2 of the query command.
- 4) Calculate the CV programming accuracy ($|U_1 - 0|$) and the CV readback accuracy ($|U_2 - U_1|$). Compare them with the specified specifications in Table 2-34.

4. Measure the CV programming and readback accuracy (take CH1 as an example in this place) when the output voltage is the rated output value.

- 1) Send the following command via the remote interface to select the channel to be tested (namely the current channel) and set the voltage and current of this channel (please refer to Table 2-34).

```
:APPL CH1,8,5.3      /*Select CH1 as the current channel and set the
```


voltage and current of this channel to 8V and 5.3A respectively*/

Notes:

- The above command is only applicable to the multi-channel models of DP800. You can also send the `:INST:NSEL 1` (or `:INST CH1`) command to select CH1 as the current channel, the `:SOUR1:VOLT 8` command to set the voltage of CH1 to 8V and the `:SOUR1:CURREN 5.3` command to set the current of CH1 to 5.3A.
 - For the single channel model with multiple ranges of DP800 series (DP811A/DP811), you can send the `:OUTP:RANG P20V` (or `:OUTP:RANG LOW`, or `:VOLT:RANG P20V`, or `:VOLT:RANG LOW`) command to select Range1 as the current range and then send the `:VOLT 20` command to set the voltage of the channel to 20V and the `:CURR 10.5` command to set the current of the channel to 10.5A.
- 2) Make sure that the power supply is in CV mode. Read and record the reading (U_3) of the multimeter.
 - 3) Send the `:MEAS:VOLT? CH1` command via the remote interface; read and record the returned voltage value U_4 of the query command.
 - 4) Calculate the CV programming accuracy ($|U_3 - U_R|$) and the CV readback accuracy ($|U_4 - U_3|$). Compare them with the specified specifications in Table 2-34. Wherein, U_R is the rated output voltage of the channel under test.
 - 5) Send the following command via the remote interface to disable the output of the channel under test.

`:OUTP CH1,OFF` /*Disable the output of CH1*/

5. Repeat steps 1 to 4 to test the CV programming and readback accuracy of CH2 and CH3 until finishing the CV programming and readback accuracy tests of all channels.

Note: For the multi-channel models of DP800 series, please replace the “CH1” in the remote commands in steps 3 and 4 with “CH2” or “CH3” to select and set the corresponding channel.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select Range1, set the parameters of Range1 and measure the CV programming and readback accuracy of this range in steps 3 and 4. Then, repeat step 3 and step 4 to test the CV programming and readback accuracy of Range2 (please replace the "P20V" or "LOW" in the remote commands in steps 3 and 4 with "P40V" or "HIGH").
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply and multimeter according to Figure 2-2 and send the remote command (DP821A/DP821: :OUTP:SENS CH2,ON; DP811A/DP811: :OUTP:SENS CH1,ON) to turn on the Sense function of the channel under test before turning on the output of the channel under test in step 3.

Test Record Forms:

Table 2-34 DP831A CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<13mV	<35mV	<35mV
	Readback	<13mV	<25mV	<25mV
The output voltage is 0				
DP831A Setting	Voltage	0V	0V	0V
	Current	5.3A	2.1A	2.1A
Measurement Result	U ₁			
	U ₂			
	Programming: U ₁ -0			
	Readback: U ₂ -U ₁			
The output voltage is U _R ^[1]				
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U ₃			
	U ₄			
	Programming: U ₃ -U _R ^[1]			
	Readback: U ₄ -U ₃			

Note^[1]: The rated voltage of the specified channel.

Table 2-35 DP831 CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<13mV	<35mV	<35mV
	Readback	<13mV	<25mV	<25mV
The output voltage is 0				
DP831 Setting	Voltage	0V	0V	0V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_1			
	U_2			
	Programming: $ U_1-0 $			
	Readback: $ U_2-U_1 $			
The output voltage is $U_R^{[1]}$				
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_3			
	U_4			
	Programming: $ U_3-U_R^{[1]} $			
	Readback: $ U_4-U_3 $			

Note^[1]: The rated voltage of the specified channel.

Table 2-36 DP832A CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<35mV	<35mV	<10mV
	Readback	<25mV	<25mV	<10mV
The output voltage is 0				
DP832A Setting	Voltage	0V	0V	0V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_1			
	U_2			
	Programming: $ U_1-0 $			
	Readback: $ U_2-U_1 $			
The output voltage is $U_R^{[1]}$				
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_3			
	U_4			
	Programming: $ U_3-U_R^{[1]} $			
	Readback: $ U_4-U_3 $			

Note^[1]: The rated voltage of the specified channel.

Table 2-37 DP832 CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<35mV	<35mV	<10mV
	Readback	<25mV	<25mV	<10mV
The output voltage is 0				
DP832 Setting	Voltage	0V	0V	0V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_1			
	U_2			
	Programming: $ U_1-0 $			
	Readback: $ U_2-U_1 $			
The output voltage is $U_R^{[1]}$				
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_3			
	U_4			
	Programming: $ U_3-U_R^{[1]} $			
	Readback: $ U_4-U_3 $			

Note^[1]: The rated voltage of the specified channel.

Table 2-38 DP821A CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<85mV	<14mV
	Readback	<85mV	<9mV
The output voltage is 0			
DP821A Setting	Voltage	0V	0V
	Current	1.05A	10.5A
Measurement Result	U_1		
	U_2		
	Programming: $ U_1-0 $		
	Readback: $ U_2-U_1 $		
The output voltage is $U_R^{[1]}$			
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_1		
	U_2		
	Programming: $ U_3-U_R^{[1]} $		
	Readback: $ U_4-U_3 $		

Note^[1]: The rated voltage of the specified channel.

Table 2-39 DP821A CV Programming and Readback Accuracy Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<85mV	<14mV
	Readback	<85mV	<9mV
The output voltage is 0			
DP821A Setting	Voltage	0V	0V
	Current	1.05A	10.5A
Measurement Result	U_1		
	U_2		
	Programming: $ U_1-0 $		
	Readback: $ U_2-U_1 $		
The output voltage is $U_R^{[1]}$			
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_1		
	U_2		
	Programming: $ U_3-U_R^{[1]} $		
	Readback: $ U_4-U_3 $		

Note^[1]: The rated voltage of the specified channel.

Table 2-40 DP811A CV Programming and Readback Accuracy Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mV	<30mV
	Readback	<20mV	<30mV
The output voltage is 0			
DP811A Setting	Voltage	0V	0V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_1-0 $		
	Readback: $ U_2-U_1 $		
The output voltage is $U_R^{[1]}$			
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_3-U_R^{[1]} $		
	Readback: $ U_4-U_3 $		

Note^[1]: The rated voltage of the specified range.

Table 2-41 DP811 CV Programming and Readback Accuracy Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mV	<30mV
	Readback	<20mV	<30mV
The output voltage is 0			
DP811 Setting	Voltage	0V	0V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_1-0 $		
	Readback: $ U_2-U_1 $		
The output voltage is $U_R^{[1]}$			
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_3-U_R^{[1]} $		
	Readback: $ U_4-U_3 $		

Note^[1]: The rated voltage of the specified range.

Chapter 3 Constant Current Tests

Topics of this chapter:

- Preparations
- CC Load Regulation Rate (CC Load Effect)
- CC Linear Regulation Rate (CC Source Effect)
- CC Ripple and Noise (Normal Mode)
- CC Programming and Readback Accuracy

Preparations

When the power supply is in CC mode, the main parameters to be tested include CC load regulation rate, CC linear regulation rate, CC ripple and noise and CC programming and readback accuracy.

Before performing the tests, select the appropriate voltage via the “voltage selector” at the rear panel of the power supply according to the AC line voltage of the country (230V is taken as an example in all the tests in this manual). Under normal temperature (about 25°C), make connections according to Figure 3-1 or Figure 3-2 using the devices recommended in “**Recommended Test Devices**” (for CC ripple and noise test, please connect the desired devices according to Figure 2-1 or Figure 2-2). During the test process, please set the voltage of the AC power supply according to the voltage selected of the “voltage selector” at the rear panel of the power supply.

In CC tests (not including CC ripple and noise test), a current sampling resistor should be connected between the power supply under test and the electronic load serially to convert the current signal under test to voltage signal for the measurement of related parameters.

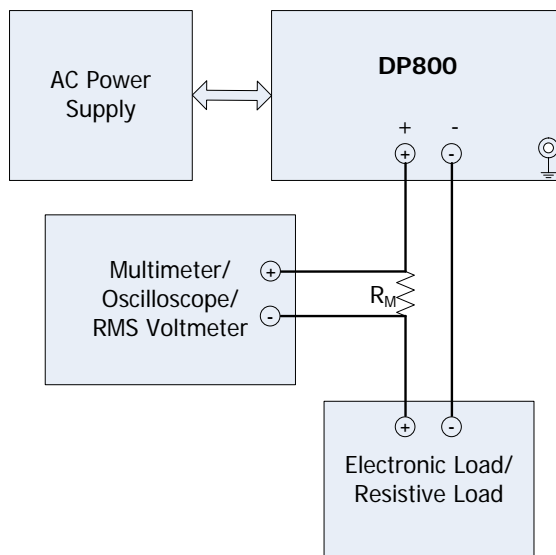


Figure 3-1 CC Test Connections

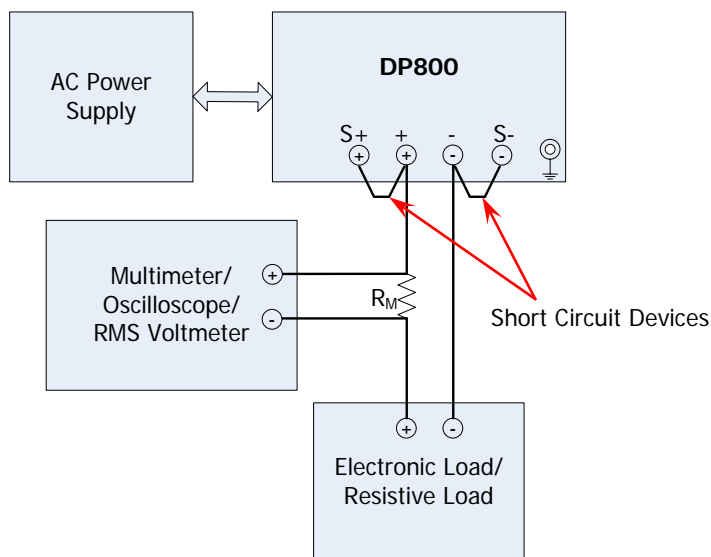


Figure 3-2 CC Test Connections (Sense)

Notes:

- During the CC tests, make connections according to Figure 3-1 for the normal channels (namely the channels that do not support the Sense function) of the DP800 series power supply. For the channels that support the Sense function (DP811A/DP811 and CH2 of DP821A/DP821), make connections according to Figure 3-2 (note to short-circuit the (S+) and (+) terminals, (S-) and (-) terminals of the channel respectively) and turn on the Sense function of the channel during the test process to measure the specifications under Sense mode.
- The R_M in the figures above is a 4-wire current sampling resistor (please select current sampling resistor with suitable resistance according to the test item and the channel to be tested). As shown in Figure 3-3, **C** represents the current measurement terminal and **S** represents the voltage measurement terminal. During the test, please make the correct connections.

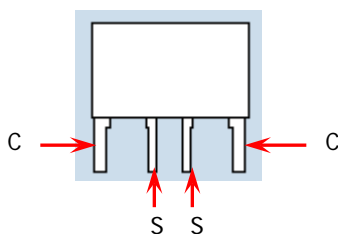


Figure 3-3 4-wire Current Sampling Resistor

CC Load Regulation Rate (CC Load Effect)

CC load regulation rate refers to the relation between the variation of the output current (caused by the load effect) and the rated output current when the power supply is under CC output mode.

DP831A is taken as an example to test the CC load regulation rate of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Load Regulation Rate, \pm (Output Percentage+Offset)	
Current	$<0.01\%+250\mu\text{A}$

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, current sampling resistor (the resistance R_M is 0.022Ω), electronic load and multimeter according to Figure 3-1. Please pay attention to the connection method of the current sampling resistor, electronic load and the channel output terminals of DP800 as well as the connection method of the current sampling resistor and multimeter. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.

2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 3-1. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.
4. Turn on the electronic load. Set the electronic load to short circuit mode. At this point, the channel under test of the power supply is in CC mode.
5. Turn on the digital multimeter; select DC voltage measurement function and set the range to "Auto". Make sure that the power supply is in CC mode. Read and record the reading (U_0 , namely the voltage of the current sampling resistor) of the multimeter.

6. Set the electronic load to work in CV mode and adjust the voltage of the electronic load to the rated output voltage (please refer to Table 1-1) of the channel (range) under test. At this point, the channel under test of the power supply is still in CC mode and is near full load output. Read and record the reading (U_1) of the multimeter.
7. Calculate the current variation ($|U_1/R_M - U_0/R_M|$) and compare it with the specified specification in Table 3-1.
8. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
9. Repeat steps 1 to 8 to test the CC load regulation rates of CH2 and CH3 until finishing the CC load regulation rate tests of all channels.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform steps 4 to 8 to test the CC load regulation rate of this range. Then, repeat steps 3 to 8 to test the CC load regulation rate of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, current sampling resistor, electronic load and multimeter according to Figure 3-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 3-1 DP831A CC Load Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[1]} - U_0/R_M^{[1]} $			

Note^[1]: $R_M=0.022\Omega$.

Table 3-2 DP831 CC Load Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[1]}-U_0/R_M^{[1]} $			

Note^[1]: $R_M=0.022\Omega$.

Table 3-3 DP832A CC Load Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[1]}-U_0/R_M^{[1]} $			

Note^[1]: $R_M=0.022\Omega$.

Table 3-4 DP832 CC Load Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[1]}-U_0/R_M^{[1]} $			

Note^[1]: $R_M=0.022\Omega$.

Table 3-5 DP821A CC Load Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[1]}-U_0/R_M^{[1]} $		

Note^[1]: $R_M=0.022\Omega$.

Table 3-6 DP821 CC Load Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[1]} - U_0/R_M^{[1]} $		

Note^[1]: $R_M=0.022\Omega$.

Table 3-7 DP811A CC Load Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750 μ A
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[1]} - U_0/R_M^{[1]} $		

Note^[1]: $R_M=0.022\Omega$.

Table 3-8 DP811 CC Load Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750 μ A
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[1]} - U_0/R_M^{[1]} $		

Note^[1]: $R_M=0.022\Omega$.

CC Linear Regulation Rate (CC Source Effect)

CC linear regulation rate refers to the relation between the variation of the output current (caused by the variation of the input power) and the rated output current when the power supply is under CC output mode.

DP831A is taken as an example to test the CC linear regulation rate of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Linear Regulation Rate, \pm (Output Percentage+Offset)	
Current	<0.01%+250 μ A

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, current sampling resistor (the resistance R_M is 0.022 Ω), electronic load and multimeter according to Figure 3-1. Please pay attention to the connection method of the current sampling resistor, electronic load and the channel output terminals of DP800 as well as the connection method of the current sampling resistor and multimeter. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.

Note: Set the voltage selector (100, 115 or 230) at the rear panel of DP800 according to your need and make sure that the fuse currently installed matches the actual input voltage (please refer to Table 2-9). As the test methods when selecting different voltages are the same, 230V is taken as an example for illustration.

2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 3-9. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.

4. Turn on the electronic load; set the electronic load to work in CV mode and adjust the voltage of the electronic load to the rated output voltage (please refer to Table 1-1) of the channel (range) under test.
5. Turn on the digital multimeter; select DC voltage measurement function and set the range to "Auto". Make sure that the power supply is in CC mode. Read and record the reading (U_0 , namely the voltage of the current sampling resistor) of the multimeter.
6. Adjust the AC power supply to undervoltage state (namely the amplitude reduces by 10%, refer to Table 2-9); read and record the reading (U_1) of the multimeter. Adjust the AC power supply to overvoltage state (namely the amplitude increases by 10%, refer to Table 2-9); read and record the reading (U_2) of the multimeter.

Note: The upper limit of the overvoltage of DP800 series is 250Vac.

7. Calculate the voltage variations (namely the CC source effect, $|U_1 - U_0|/R_M$ and $|U_2 - U_0|/R_M$) and compare them with the specified specifications in Table 3-9.
8. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
9. Repeat steps 1 to 8 to test the CC linear regulation rates of CH2 and CH3 until finishing the CC linear regulation rate tests of all channels.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform step 4 to step 8 to test the CC linear regulation rate of this range. Then, repeat step 3 to step 8 to test the CC linear regulation rate of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, current sampling resistor, electronic load and multimeter according to Figure 3-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 3-9 DP831A CC Linear Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 /R_M^{[1]}$			
	$ U_2-U_0 /R_M^{[1]}$			

Note^[1]: $R_M=0.022\Omega$.

Table 3-10 DP831 CC Linear Regulation Rate Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 /R_M^{[1]}$			
	$ U_2-U_0 /R_M^{[1]}$			

Note^[1]: $R_M=0.022\Omega$.

Table 3-11 DP832A CC Linear Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 /R_M^{[1]}$			
	$ U_2-U_0 /R_M^{[1]}$			

Note^[1]: $R_M=0.022\Omega$.

Table 3-12 DP832 CC Linear Regulation Rate Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1-U_0 /R_M^{[1]}$			
	$ U_2-U_0 /R_M^{[1]}$			

Note^[1]: $R_M=0.022\Omega$.

Table 3-13 DP821A CC Linear Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 /R_M^{[1]}$		
	$ U_2-U_0 /R_M^{[1]}$		

Note^[1]: $R_M=0.022\Omega$.

Table 3-14 DP821 CC Linear Regulation Rate Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 /R_M^{[1]}$		
	$ U_2-U_0 /R_M^{[1]}$		

Note^[1]: $R_M=0.022\Omega$.

Table 3-15 DP811A CC Linear Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 /R_M^{[1]}$		
	$ U_2-U_0 /R_M^{[1]}$		

Note^[1]: $R_M=0.022\Omega$.

Table 3-16 DP811 CC Linear Regulation Rate Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1-U_0 /R_M^{[1]}$		
	$ U_2-U_0 /R_M^{[1]}$		

Note^[1]: $R_M=0.022\Omega$.

CC Ripple and Noise (Normal Mode)

When the power supply is working in CC mode, the ripple and noise are usually expressed in RMS value form.

DP831A is taken as an example to test the CC ripple and noise of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Ripple and Noise (20 Hz to 20 MHz)	
Normal Mode Current	<2mArms

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, resistive load and RMS voltmeter according to Figure 2-1. Both the resistive load and RMS voltmeter are connected with the channel output terminals of DP800; please refer to “**Test Precautions**” for the connection method. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3.

Note:

- Do not connect the negative terminal of the output terminal of the channel to be tested to the shielding ground; otherwise, a ground loop would be formed. In Figure 2-3, the connection in figure A forms a ground loop while figure B shows the correct connection.
- Please ensure to test the CC ripple and noise of DP800 under full load condition. Refer to Table 3-17 for the resistance of the resistive load.

2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Turn on DP800 and press the channel selecting key at the front panel to select CH1 as the channel to be tested. Set the voltage and current of the channel under test according to Table 3-17. Then, press the **On/Off** key corresponding to the channel under test to enable the output of the channel.
4. Turn on the RMS voltmeter and select the AC voltage random measurement mode (SETACV RNDM). Make sure that the power supply is in CC mode. Read

and record the RMS value (V_{rms}) measured by the RMS voltmeter.

Note: The measurement wires of the RMS voltmeter should be twisted together to minimize the effect of the space radiation noise on the test as much as possible.

5. Calculate the CC ripple and noise (V_{rms}/R_L) and compare it with the specified specification in Table 3-17.
6. Press the **On/Off** key corresponding to the channel under test at the front channel to disable the output of the channel under test.
7. Repeat steps 1 to 6 to test the CC ripple and noise (normal mode) of CH2 and CH3 until finishing the CC ripple and noise tests of all channels.

Notes:

- During the CC ripple and noise test, please pay attention to shield the effect of the environmental space radiation noise on the test effectively.
- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), please first select a range and set the corresponding parameters of this range in step 3 and then perform step 4 to step 6 to test the CC ripple and noise of this range. Then, repeat step 3 to step 6 to test the CC ripple and noise of the other range.
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, resistive load and RMS voltmeter according to Figure 2-2 and turn on the Sense function of the channel after selecting the current channel in step 3.

Test Record Forms:

Table 3-17 DP831A CC Ripple and Noise Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2mArms		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	RMS value (V_{rms})			
	V_{rms}/R_L			

Table 3-18 DP831 CC Ripple and Noise Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2mArms		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

Table 3-19 DP832A CC Ripple and Noise Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<2mArms		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

Table 3-20 DP832 CC Ripple and Noise Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<2mArms		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

Table 3-21 DP821A CC Ripple and Noise Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<2mArms	
Resistive Load R_L		60 Ω	0.8 Ω
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

Table 3-22 DP821 CC Ripple and Noise Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<2mArms	
Resistive Load R_L		60 Ω	0.8 Ω
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

Table 3-23 DP811A CC Ripple and Noise Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<2mArms	
Resistive Load R_L		2 Ω	8 Ω
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

Table 3-24 DP811 CC Ripple and Noise Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<2mArms	
Resistive Load R_L		2 Ω	8 Ω
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

CC Programming and Readback Accuracy

CC programming accuracy refers to the error between the current setting value of the channel and the actual output current value when the power supply is in CC mode; CC readback accuracy refers to the error between the actual output current value and the readback current value when the power supply is in CC mode.

DP831A is taken as an example to test the CC programming and readback accuracy of DP800 series in the following section.

Note: During the actual test, please select the corresponding test record form according to the model of the DP800 power supply under test to set the corresponding parameters, record and calculate the corresponding specifications.

Specification:

Annual Accuracy ^[1] (25℃±5℃)± (Output Percentage+Offset)			
Channel		Programming	Readback
DP831A/DP831	CH1	0.2%+10mA	0.2%+10mA
	CH2	0.2%+5mA	0.1%+5mA
	CH3	0.2%+5mA	0.1%+5mA
DP832A/DP832	CH1	0.2%+5mA	0.15%+5mA
	CH2	0.2%+5mA	0.15%+5mA
	CH3	0.2%+5mA	0.15%+5mA
DP821A/DP821	CH1	0.2%+10mA	0.15%+10mA
	CH2	0.2%+10mA	0.15%+10mA
DP811A/DP811	CH1	0.1%+10mA	0.1%+10mA

Note^[1]: The accuracy parameters are acquired via calibration under 25℃ after 1-hour warm-up.

Test Procedures:

1. Turn off DP800. Connect DP800, AC power supply, current sampling resistor (the resistance R_M is 0.022Ω) and multimeter according to Figure 3-1. Please pay attention to the connection method of the current sampling resistor and the channel output terminals of DP800 as well as the connection method of the current sampling resistor and multimeter. Here, CH1 is taken as an example and the connection method is also applicable to CH2 and CH3. Then, connect the power supply with PC (take the connection via USB cable as an example) via the remote interfaces (USB, GPIB, LAN).
2. Turn on the AC power supply; set its voltage to 230V and frequency to 50Hz.

Note: The voltage setting of the AC power supply in this step should be in accordance with the value selected by the voltage selector at the rear panel of DP800.

3. Measure the CC programming and readback accuracy (take CH1 as an example in this place) when the output current is 0A.

- 1) Turn on DP800. Send the following commands via the remote interface to select the channel to be tested (namely the current channel), set the voltage and current of this channel (please refer to Table 3-25) as well as enable the output of this channel.

```
:APPL CH1,8.4,0 /*Select CH1 as the current channel and set the
                  voltage and current of this channel to 8.4V and
                  0A respectively*/
:OUTP CH1,ON /*Enable the output of CH1*/
```

Notes:

- The above commands are only applicable to the multi-channel models of DP800. You can also send the `:INST:NSEL 1` (or `:INST CH1`) command to select CH1 as the current channel, the `:SOUR1:VOLT 8.4` command to set the voltage of CH1 to 8.4V and the `:SOUR1:CURREN 0` command to set the current of CH1 to 0A.
 - For the single channel model with multiple ranges of DP800 series (DP811A/DP811), you can send the `:OUTP:RANG P20V` (or `:OUTP:RANG LOW`, or `:VOLT:RANG P20V`, or `:VOLT:RANG LOW`) command to select Range1 as the current range and then send the `:VOLT 21` command to set the voltage of the channel to 21V and the `:CURREN 0` command to set the current of the channel to 0A.
- 2) Turn on the digital multimeter; select DC voltage measurement function and set the range to "Auto". Make sure that the power supply is in CC mode. Read and record the reading (U_1) of the multimeter. Calculate the current value $I_1 = U_1 / R_M$.
 - 3) Send the `:MEAS:CURREN? CH1` command via the remote interface; read and record the returned current value I_2 of the query command.
 - 4) Calculate the CC programming accuracy ($|I_1 - 0|$) and the CC readback accuracy ($|I_2 - I_1|$). Compare them with the specified specifications in Table 3-25.

4. Measure the CC programming and readback accuracy (take CH1 as an example in this place) when the output current is the rated output value.

- 1) Send the following command via the remote interface to select the channel to be tested (namely the current channel) and set the voltage and current of this channel (please refer to Table 3-25).

```
:APPL CH1,8.4,5 /* Select CH1 as the current channel and set the
                  voltage and current of this channel to 8.4V and
                  5A respectively*/
```

Notes:

- The above command is only applicable to the multi-channel models of DP800. You can also send the `:INST:NSEL 1` (or `:INST CH1`) command

to select CH1 as the current channel, the `:SOUR1:VOLT 8.4` command to set the voltage of CH1 to 8.4V and the `:SOUR1:CURREN 5` command to set the current of CH1 to 5A.

- For the single channel model with multiple ranges of DP800 series (DP811A/DP811), you can send the `:OUTP:RANG P20V` (or `:OUTP:RANG LOW`, or `:VOLT:RANG P20V`, or `:VOLT:RANG LOW`) command to select Range1 as the current range and then send the `:VOLT 21` command to set the voltage of the channel to 21V and the `:CURREN 10` command to set the current of the channel to 10A.
- 2) Make sure that the power supply is in CC mode. Read and record the reading (U_3) of the multimeter. Calculate the current value $I_3 = U_3 / R_M$.
 - 3) Send the `:MEAS:CURREN? CH1` command via the remote interface; read and record the returned current value I_4 of the query command.
 - 4) Calculate the CC programming accuracy ($|I_3 - I_R|$) and the CC readback accuracy ($|I_4 - I_3|$). Compare them with the specified specifications in Table 3-25. Wherein, I_R is the rated output current of the channel under test.
 - 5) Send the following command via the remote interface to disable the output of the channel under test.

`:OUTP CH1,OFF` /*Disable the output of CH1*/

5. Repeat steps 1 to 4 to test the CC programming and readback accuracy of CH2 and CH3 until finishing the CC programming and readback accuracy tests of all channels.

Note: For the multi-channel models of DP800 series, please replace the "CH1" in the remote commands in steps 3 and 4 with "CH2" or "CH3" to select and set the corresponding channel.

Notes:

- For the single channel model with multiple ranges of DP800 series (DP811A), please first select Range1, set the parameters of Range1 and measure the CC programming and readback accuracy of this range in steps 3 and 4. Then, repeat steps 3 and 4 to test the CC programming and readback accuracy of Range2 (please replace the "P20V" or "LOW" in the remote commands in steps 3 and 4 with "P40V" or "HIGH").
- For the channels that support the Sense function of DP800 series, please connect DP800, AC power supply, current sampling resistor and multimeter according to Figure 3-2 and send the remote command (DP821A: `:OUTP:SENS CH2,ON`; DP811A: `:OUTP:SENS CH1,ON`) to turn on the Sense function of the channel under test before turning on the output of the channel under test in step 3.

Test Record Forms:

Table 3-25 DP831A CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<20mA	<9mA	<9mA
	Readback	<20mA	<7mA	<7mA
The output current is 0				
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1/R_M^{[1]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[2]}$				
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_3			
	$I_3 = U_3/R_M^{[1]}$			
	I_4			
	Programming: $ I_3 - I_R^{[2]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified channel.

Table 3-26 DP831 CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<20mA	<9mA	<9mA
	Readback	<20mA	<7mA	<7mA
The output current is 0				
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1 / R_M^{[1]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[2]}$				
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_3			
	$I_3 = U_3 / R_M^{[1]}$			
	I_4			
	Programming: $ I_3 - I_R^{[2]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified channel.

Table 3-27 DP832A CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<11mA		
	Readback	<9.5mA		
The output current is 0				
DP832A Setting	Voltage	32V	32V	5.3V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1 / R_M^{[1]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[2]}$				
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_3			
	$I_3 = U_3 / R_M^{[1]}$			
	I_4			
	Programming: $ I_3 - I_R^{[2]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: $R_M = 0.022\Omega$.Note^[2]: The rated current of the specified channel.

Table 3-28 DP832 CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<11mA		
	Readback	<9.5mA		
The output current is 0				
DP832 Setting	Voltage	32V	32V	5.3V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1 / R_M^{[1]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[2]}$				
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_3			
	$I_3 = U_3 / R_M^{[1]}$			
	I_4			
	Programming: $ I_3 - I_R^{[2]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified channel.

Table 3-29 DP821A CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<12mA	<30mA
	Readback	<11.5mA	<25mA
The output current is 0			
DP821A Setting	Voltage	63V	8.4V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1 / R_M^{[1]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[2]}$			
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_3		
	$I_3 = U_3 / R_M^{[1]}$		
	I_4		
	Programming: $ I_3 - I_R^{[2]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified channel.

Table 3-30 DP821 CC Programming and Readback Accuracy Test Record Form

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<12mA	<30mA
	Readback	<11.5mA	<25mA
The output current is 0			
DP821 Setting	Voltage	63V	8.4V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1 / R_M^{[1]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[2]}$			
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_3		
	$I_3 = U_3 / R_M^{[1]}$		
	I_4		
	Programming: $ I_3 - I_R^{[2]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified channel.

Table 3-31 DP811A CC Programming and Readback Accuracy Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mA	<15mA
	Readback	<20mA	<15mA
The output current is 0			
DP811A Setting	Voltage	21V	42V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1/R_M^{[1]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[2]}$			
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_3		
	$I_3 = U_3/R_M^{[1]}$		
	I_4		
	Programming: $ I_3 - I_R^{[2]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified range.

Table 3-32 DP811 CC Programming and Readback Accuracy Test Record Form

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mA	<15mA
	Readback	<20mA	<15mA
The output current is 0			
DP811 Setting	Voltage	21V	42V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1 / R_M^{[1]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[2]}$			
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_3		
	$I_3 = U_3 / R_M^{[1]}$		
	I_4		
	Programming: $ I_3 - I_R^{[2]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: $R_M = 0.022\Omega$.

Note^[2]: The rated current of the specified range.

Appendix

Appendix A: Test Result Record Forms

DP831A Performance Verification Test Record Form

RIGOL DP831A Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

CV Linear Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 $			
	$ U_2 - U_0 $			

CV Ripple and Noise

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<350 μ Vrms/3mVpp		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Transient Response Time

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<50 μ s		
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Electronic Load Current Setting	CCDH1	5A	2A	2A
	CCDH2	2.5A	1A	1A
Measurement Result	t			

CV Programming and Readback Accuracy

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<13mV	<35mV	<35mV
	Readback	<13mV	<25mV	<25mV
The output voltage is 0				
DP831A Setting	Voltage	0V	0V	0V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_1			
	U_2			
	Programming: $ U_1-0 $			
	Readback: $ U_2-U_1 $			
The output voltage is $U_R^{[1]}$				
DP831A Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_3			
	U_4			
	Programming: $ U_3-U_R^{[1]} $			
	Readback: $ U_4-U_3 $			

CC Load Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[2]}-U_0/R_M^{[2]} $			

CC Linear Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 /R_M^{[2]}$			
	$ U_2 - U_0 /R_M^{[2]}$			

CC Ripple and Noise

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2mArms		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

CC Programming and Readback Accuracy

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<20mA	<9mA	<9mA
	Readback	<20mA	<7mA	<7mA
The output current is 0				
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1/R_M^{[2]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[3]}$				
DP831A Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_3			
	$I_3 = U_3/R_M^{[2]}$			
	I_4			
	Programming: $ I_3 - I_R^{[3]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP831 Performance Verification Test Record Form

RIGOL DP831 Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

CV Linear Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2.8mV	<5mV	<5mV
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 $			
	$ U_2 - U_0 $			

CV Ripple and Noise

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<350 μ Vrms/3mVpp		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Transient Response Time

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<50μs		
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Electronic Load Current Setting	CCDH1	5A	2A	2A
	CCDH2	2.5A	1A	1A
Measurement Result	t			

CV Programming and Readback Accuracy

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<13mV	<35mV	<35mV
	Readback	<13mV	<25mV	<25mV
The output voltage is 0				
DP831 Setting	Voltage	0V	0V	0V
	Current	5.3A	2.1A	2.1A
Measurement Result	U ₁			
	U ₂			
	Programming: U ₁ -0			
	Readback: U ₂ -U ₁			
The output voltage is U _R ^[1]				
DP831 Setting	Voltage	8V	30V	-30V
	Current	5.3A	2.1A	2.1A
Measurement Result	U ₃			
	U ₄			
	Programming: U ₃ -U _R ^[1]			
	Readback: U ₄ -U ₃			

CC Load Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750μA	<450μA	<450μA
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U ₀			
	U ₁			
	U ₁ /R _M ^[2] -U ₀ /R _M ^[2]			

CC Linear Regulation Rate

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<750 μ A	<450 μ A	<450 μ A
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 /R_M^{[2]}$			
	$ U_2 - U_0 /R_M^{[2]}$			

CC Ripple and Noise

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification		<2mArms		
Resistive Load R_L		1.6 Ω	15 Ω	15 Ω
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	RMS value (V_{rms})			
	V_{rms}/R_L			

CC Programming and Readback Accuracy

Channel		CH1 (8V/5A)	CH2 (30V/2A)	CH3 (-30V/2A)
Specification	Programming	<20mA	<9mA	<9mA
	Readback	<20mA	<7mA	<7mA
The output current is 0				
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1 = U_1/R_M^{[2]}$			
	I_2			
	Programming: $ I_1 - 0 $			
	Readback: $ I_2 - I_1 $			
The output current is $I_R^{[3]}$				
DP831 Setting	Voltage	8.4V	32V	-32V
	Current	5A	2A	2A
Measurement Result	U_3			
	$I_3 = U_3/R_M^{[2]}$			
	I_4			
	Programming: $ I_3 - I_R^{[3]} $			
	Readback: $ I_4 - I_3 $			

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP832A Performance Verification Test Record Form

RIGOL DP832A Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

CV Linear Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 $			
	$ U_2 - U_0 $			

CV Ripple and Noise

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<350 μ Vrms/3mVpp		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Transient Response Time

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<50 μ s		
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Electronic Load Current Setting	CCDH1	3A	3A	3A
	CCDH2	1.5A	1.5A	1.5A
Measurement Result	t			

CV Programming and Readback Accuracy

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<35mV	<35mV	<10mV
	Readback	<25mV	<25mV	<10mV
The output voltage is 0				
DP832A Setting	Voltage	0V	0V	0V
	Current	3.2A	3.2A	3.2A
Measurement Result	U ₁			
	U ₂			
	Programming: U ₁ -0			
	Readback: U ₂ -U ₁			
The output voltage is U _R ^[1]				
DP832A Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U ₃			
	U ₄			
	Programming: U ₃ -U _R ^[1]			
	Readback: U ₄ -U ₃			

CC Load Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $			

CC Linear Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 /R_M^{[2]}$			
	$ U_2 - U_0 /R_M^{[2]}$			

CC Ripple and Noise

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<2mArms		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

CC Programming and Readback Accuracy

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<11mA		
	Readback	<9.5mA		
The output current is 0				
DP832A Setting	Voltage	32V	32V	5.3V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1=U_1/R_M^{[2]}$			
	I_2			
	Programming: $ I_1-0 $			
	Readback: $ I_2-I_1 $			
The output current is $I_R^{[3]}$				
DP832A Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_3			
	$I_3=U_3/R_M^{[2]}$			
	I_4			
	Programming: $ I_3-I_R^{[3]} $			
	Readback: $ I_4-I_3 $			

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP832 Performance Verification Test Record Form

RIGOL DP832 Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	$ U_1 - U_0 $			

CV Linear Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<5mV	<5mV	<2.5mV
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 $			
	$ U_2 - U_0 $			

CV Ripple and Noise

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<350 μ Vrms/3mVpp		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	Peak-peak value (Vpp)			
	RMS value (Vrms)			

Transient Response Time

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<50 μ s		
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Electronic Load Current Setting	CCDH1	3A	3A	3A
	CCDH2	1.5A	1.5A	1.5A
Measurement Result	t			

CV Programming and Readback Accuracy

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<35mV	<35mV	<10mV
	Readback	<25mV	<25mV	<10mV
The output voltage is 0				
DP832 Setting	Voltage	0V	0V	0V
	Current	3.2A	3.2A	3.2A
Measurement Result	U ₁			
	U ₂			
	Programming: U ₁ -0			
	Readback: U ₂ -U ₁			
The output voltage is U _R ^[1]				
DP832 Setting	Voltage	30V	30V	5V
	Current	3.2A	3.2A	3.2A
Measurement Result	U ₃			
	U ₄			
	Programming: U ₃ -U _R ^[1]			
	Readback: U ₄ -U ₃			

CC Load Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $			

CC Linear Regulation Rate

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<550 μ A		
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_0			
	U_1			
	U_2			
	$ U_1 - U_0 /R_M^{[2]}$			
	$ U_2 - U_0 /R_M^{[2]}$			

CC Ripple and Noise

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification		<2mArms		
Resistive Load R_L		10 Ω	10 Ω	1.6 Ω
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	RMS value (Vrms)			
	Vrms/ R_L			

CC Programming and Readback Accuracy

Channel		CH1 (30V/3A)	CH2 (30V/3A)	CH3 (5V/3A)
Specification	Programming	<11mA		
	Readback	<9.5mA		
The output current is 0				
DP832 Setting	Voltage	32V	32V	5.3V
	Current	0A	0A	0A
Measurement Result	U_1			
	$I_1=U_1/R_M^{[2]}$			
	I_2			
	Programming: $ I_1-0 $			
	Readback: $ I_2-I_1 $			
The output current is $I_R^{[3]}$				
DP832 Setting	Voltage	32V	32V	5.3V
	Current	3A	3A	3A
Measurement Result	U_3			
	$I_3=U_3/R_M^{[2]}$			
	I_4			
	Programming: $ I_3-I_R^{[3]} $			
	Readback: $ I_4-I_3 $			

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP821A Performance Verification Test Record Form

RIGOL DP821A Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

CV Linear Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 $		
	$ U_2 - U_0 $		

CV Ripple and Noise

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ Vrms/3mVpp	
Resistive Load R_L		60 Ω	0.8 Ω
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Transient Response Time

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<50 μ s	
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Electronic Load Current Setting	CCDH1	1A	10A
	CCDH2	0.5A	5A
Measurement Result	t		

CV Programming and Readback Accuracy

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<85mV	<14mV
	Readback	<85mV	<9mV
The output voltage is 0			
DP821A Setting	Voltage	0V	0V
	Current	1.05A	10.5A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₁ -0		
	Readback: U ₂ -U ₁		
The output voltage is U _R ^[1]			
DP821A Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₃ -U _R ^[1]		
	Readback: U ₄ -U ₃		

CC Load Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $		

CC Linear Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[2]}$		
	$ U_2 - U_0 /R_M^{[2]}$		

CC Ripple and Noise

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<2mArms	
Resistive Load R_L		60 Ω	0.8 Ω
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

CC Programming and Readback Accuracy

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<12mA	<30mA
	Readback	<11.5mA	<25mA
The output current is 0			
DP821A Setting	Voltage	63V	8.4V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1 / R_M^{[2]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[3]}$			
DP821A Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_3		
	$I_3 = U_3 / R_M^{[2]}$		
	I_4		
	Programming: $ I_3 - I_R^{[3]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP821 Performance Verification Test Record Form

RIGOL DP821 Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

CV Linear Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<8mV	<2.8mV
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 $		
	$ U_2 - U_0 $		

CV Ripple and Noise

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ Vrms/3mVpp	
Resistive Load R_L		60 Ω	0.8 Ω
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Transient Response Time

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<50 μ s	
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Electronic Load Current Setting	CCDH1	1A	10A
	CCDH2	0.5A	5A
Measurement Result	t		

CV Programming and Readback Accuracy

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<85mV	<14mV
	Readback	<85mV	<9mV
The output voltage is 0			
DP821 Setting	Voltage	0V	0V
	Current	1.05A	10.5A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₁ -0		
	Readback: U ₂ -U ₁		
The output voltage is U _R ^[1]			
DP821 Setting	Voltage	60V	8V
	Current	1.05A	10.5A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₃ -U _R ^[1]		
	Readback: U ₄ -U ₃		

CC Load Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $		

CC Linear Regulation Rate

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<350 μ A	<1.25mA
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[2]}$		
	$ U_2 - U_0 /R_M^{[2]}$		

CC Ripple and Noise

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification		<2mArms	
Resistive Load R_L		60 Ω	0.8 Ω
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

CC Programming and Readback Accuracy

Channel		CH1 (60V/1A)	CH2 (8V/10A)
Specification	Programming	<12mA	<30mA
	Readback	<11.5mA	<25mA
The output current is 0			
DP821 Setting	Voltage	63V	8.4V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1/R_M^{[2]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[3]}$			
DP821 Setting	Voltage	63V	8.4V
	Current	1A	10A
Measurement Result	U_3		
	$I_3 = U_3/R_M^{[2]}$		
	I_4		
	Programming: $ I_3 - I_R^{[3]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: The rated voltage of the specified channel.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified channel.

DP811A Performance Verification Test Record Form

RIGOL DP811A Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

CV Linear Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[1]}$		
	$ U_2 - U_0 /R_M^{[1]}$		

CV Ripple and Noise

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<350μVrms/3mVpp	
Resistive Load R_L		2Ω	8Ω
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Transient Response Time

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<50 μ s	
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Electronic Load Current Setting	CCDH1	10A	5A
	CCDH2	5A	2.5A
Measurement Result	t		

CV Programming and Readback Accuracy

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mV	<30mV
	Readback	<20mV	<30mV
The output voltage is 0			
DP811A Setting	Voltage	0V	0V
	Current	10.5A	5.3A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₁ -0		
	Readback: U ₂ -U ₁		
The output voltage is U _R ^[1]			
DP811A Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U ₁		
	U ₂		
	Programming: U ₃ -U _R ^[1]		
	Readback: U ₄ -U ₃		

CC Load Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $		

CC Linear Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[2]}$		
	$ U_2 - U_0 /R_M^{[2]}$		

CC Ripple and Noise

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<2mArms	
Resistive Load R_L		2Ω	8Ω
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

CC Programming and Readback Accuracy

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mA	<15mA
	Readback	<20mA	<15mA
The output current is 0			
DP811A Setting	Voltage	21V	42V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1/R_M^{[2]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[3]}$			
DP811A Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_3		
	$I_3 = U_3/R_M^{[2]}$		
	I_4		
	Programming: $ I_3 - I_R^{[3]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: The rated voltage of the specified range.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified range.

DP811 Performance Verification Test Record Form

RIGOL DP811 Programmable Linear DC Power Supply Performance Verification Test Record Form

CV Load Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<4mV	<6mV
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_0		
	U_1		
	$ U_1 - U_0 $		

CV Linear Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[1]}$		
	$ U_2 - U_0 /R_M^{[1]}$		

CV Ripple and Noise

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<350μVrms/3mVpp	
Resistive Load R_L		2Ω	8Ω
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	Peak-peak value (Vpp)		
	RMS value (Vrms)		

Transient Response Time

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<50 μ s	
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Electronic Load Current Setting	CCDH1	10A	5A
	CCDH2	5A	2.5A
Measurement Result	t		

CV Programming and Readback Accuracy

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mV	<30mV
	Readback	<20mV	<30mV
The output voltage is 0			
DP811 Setting	Voltage	0V	0V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_1-0 $		
	Readback: $ U_2-U_1 $		
The output voltage is $U_R^{[1]}$			
DP811 Setting	Voltage	20V	40V
	Current	10.5A	5.3A
Measurement Result	U_1		
	U_2		
	Programming: $ U_3-U_R^{[1]} $		
	Readback: $ U_4-U_3 $		

CC Load Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	$ U_1/R_M^{[2]} - U_0/R_M^{[2]} $		

CC Linear Regulation Rate

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<1.25mA	<750μA
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_0		
	U_1		
	U_2		
	$ U_1 - U_0 /R_M^{[2]}$		
	$ U_2 - U_0 /R_M^{[2]}$		

CC Ripple and Noise

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification		<2mArms	
Resistive Load R_L		2Ω	8Ω
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	RMS value (Vrms)		
	Vrms/ R_L		

CC Programming and Readback Accuracy

Range		Range1 (20V/10A)	Range2 (40V/5A)
Specification	Programming	<20mA	<15mA
	Readback	<20mA	<15mA
The output current is 0			
DP811 Setting	Voltage	21V	42V
	Current	0A	0A
Measurement Result	U_1		
	$I_1 = U_1/R_M^{[2]}$		
	I_2		
	Programming: $ I_1 - 0 $		
	Readback: $ I_2 - I_1 $		
The output current is $I_R^{[3]}$			
DP811 Setting	Voltage	21V	42V
	Current	10A	5A
Measurement Result	U_3		
	$I_3 = U_3/R_M^{[2]}$		
	I_4		
	Programming: $ I_3 - I_R^{[3]} $		
	Readback: $ I_4 - I_3 $		

Note^[1]: The rated voltage of the specified range.

Note^[2]: $R_M = 0.022\Omega$.

Note^[3]: The rated current of the specified range.

Appendix B: Specifications

The following parameters can only be guaranteed when the instrument has been operated continuously for more than 30 minutes under the specified operating temperature.

Note: Unless otherwise noted, the specifications below apply to all channels (ranges) of the specified model.

DP832A/DP831A/DP821A/DP811A Specifications

DC Output (0°C-40°C)					
Channel		Rated Value		Maximum Settable Range	
		Voltage	Current	Overvoltage Protection	Overcurrent Protection
DP831A	CH1	0V~8V	0A~5A	1mV~8.8V	0.1mA~5.5A
	CH2	0V~30V	0A~2A	1mV~33V	0.1mA~2.2A
	CH3	-30V~0V	0A~2A	-1mV~-33V	0.1mA~2.2A
DP832A	CH1	0V~30V	0A~3A	1mV~33V	1mA~3.3A
	CH2	0V~30V	0A~3A	1mV~33V	1mA~3.3A
	CH3	0V~5V	0A~3A	1mV~5.5V	1mA~3.3A
DP821A	CH1	0V~60V	0A~1A	1mV~66V	0.1mA~1.1A
	CH2	0V~8V	0A~10A	1mV~8.8V	1mA~11A
DP811A	Range1	0V~20V	0A~10A	1mV~22V	0.1mA~11A
	Range2	0V~40V	0A~5A	1mV~44V	0.1mA~5.5A

Load Regulation rate, \pm (Output Percentage+Offset)	
Voltage	<0.01%+2mV
Current	<0.01%+250 μ A

Linear Regulation Rate, \pm (Output Percentage+Offset)	
Voltage	<0.01%+2mV
Current	<0.01%+250 μ A

Ripple and Noise (20 Hz to 20 MHz)	
Normal Mode Voltage	DP832A/DP831A/DP821A: <350 μ Vrms/2mVpp DP811A: <350 μ Vrms/3mVpp
Normal Mode Current	<2mArms

Annual Accuracy ^[1] (25°C±5°C) ±(Output Percentage+Offset)					
Channel		Programming		Readback	
		Voltage	Current	Voltage	Current
DP831A	CH1	0.1%+5mV	0.2%+10mA	0.1%+5mV	0.2%+10mA
	CH2	0.05%+20mV	0.2%+5mA	0.05%+10mV	0.1%+5mA
	CH3	0.05%+20mV	0.2%+5mA	0.05%+10mV	0.1%+5mA
DP832A	CH1	0.05%+20mV	0.2%+5mA	0.05%+10mV	0.15%+5mA
	CH2	0.05%+20mV	0.2%+5mA	0.05%+10mV	0.15%+5mA
	CH3	0.1%+5mV	0.2%+5mA	0.1%+5mV	0.15%+5mA
DP821A	CH1	0.1%+25mV	0.2%+10mA	0.1%+25mV	0.15%+10mA
	CH2	0.05%+10mV	0.2%+10mA	0.05%+5mV	0.15%+10mA
DP811A	CH1	0.05%+10mV	0.1%+10mA	0.05%+10mV	0.1%+10mA

Resolution							
Channel		Programming		Readback		Display	
		Voltage	Current	Voltage	Current	Voltage	Current
DP831A	CH1	1mV	0.3mA	0.1mV	0.1mA	1mV	1mA
	CH2	1mV	0.1mA	0.1mV	0.1mA	1mV	1mA
	CH3	1mV	0.1mA	0.1mV	0.1mA	1mV	1mA
DP832A	CH1	1mV	1mA	0.1mV	0.1mA	1mV	1mA
	CH2	1mV	1mA	0.1mV	0.1mA	1mV	1mA
	CH3	1mV	1mA	0.1mV	0.1mA	1mV	1mA
DP821A	CH1	10mV	0.1mA	1mV	0.1mA	1mV	0.1mA
	CH2	1mV	1mA	1mV	1mA	1mV	1mA
DP811A	CH1	1mV	0.5mA	0.1mV	0.1mA	1mV	1mA

Transient Response Time

Less than 50μs for output voltage to recover to within 15 mV following a change in output current from full load to half load or vice versa.

Command Processing Time^[2]

<118ms

Temperature Coefficient per°C (Output Percentage+Offset)			
Channel		Voltage	Current
DP831A	CH1	0.01%+2mV	0.02%+3mA
	CH2	0.01%+2mV	0.02%+3mA
	CH3	0.01%+2mV	0.02%+3mA
DP832A	CH1	0.01%+5mV	0.01%+2mA
	CH2	0.01%+5mV	0.01%+2mA
	CH3	0.01%+2mV	0.01%+2mA
DP821A	CH1	0.01%+3mV	0.02%+3mA
	CH2	0.01%+3mV	0.02%+3mA
DP811A	CH1	0.01%+3mV	0.02%+3mA

Stability ^[3] , ± (Output Percentage+Offset)			
Channel		Voltage	Current
DP831A	CH1	0.03%+1mV	0.1%+3mA
	CH2	0.02%+2mV	0.05%+1mA
	CH3	0.02%+2mV	0.05%+1mA
DP832A	CH1	0.02%+2mV	0.05%+2mA
	CH2	0.02%+2mV	0.05%+2mA
	CH3	0.01%+1mV	0.05%+2mA
DP821A	CH1	0.02%+1mV	0.1%+1mA
	CH2	0.02%+1mV	0.1%+1mA
DP811A	CH1	0.02%+1mV	0.1%+1mA

Voltage Programming Control Speed (1% within the total variation range)					
Channel		Rise		Fall	
		Full Load	No Load	Full Load	No Load
DP831A	CH1	<18ms	<17ms	<20ms	<200ms
	CH2	<33ms	<36ms	<44ms	<400ms
	CH3	<35ms	<42ms	<45ms	<400ms
DP832A	CH1	<50ms	<33ms	<46ms	<400ms
	CH2	<50ms	<38ms	<46ms	<400ms
	CH3	<15ms	<14ms	<24ms	<100ms
DP821A	CH1	<92ms	<30ms	<90ms	<486ms
	CH2	<11ms	<15ms	<17ms	<154ms
DP811A	CH1	<45ms	<42ms	<51ms	<1089ms

OVP/OCF	
Accuracy ± (Output Percentage+Offset)	0.5%+0.5V/0.5%+0.5A
Activation Time	1.5ms (OVP≥3V) <10ms (OVP<3V) <10ms (OCF)

Mechanical	
Dimensions	239mm (W) x 157mm (H) x 418mm (D)
Weight	DP831A: 9.75kg DP832A: 10.5kg DP821A: 10.0kg DP811A: 10.3kg

Power	
AC Input (50Hz to 60Hz)	100Vac \pm 10%, 115Vac \pm 10%, 230Vac \pm 10% (maximum 250Vac)

I/O	
USB Device	1
USB Host	1
LAN	1 (Option)
RS232	1 (Option)
Digital IO	1 (Option)
USB-GPIB	1 (Option)
Rear output interface	Only DP811A has one

Environment	
Working Temperature	DP831A/DP832A/DP832/DP811A: Full rated value output: 0℃~40℃ Under relatively higher temperature: the linearity of the output current reduces to 50% at the highest temperature 55℃ DP821A: Full rated value output: 0℃~40℃ Under relatively higher temperature: the linearity of the output current reduces to 50% at the highest temperature 55℃ or the fuse is blown out
Storage Temperature	-40℃~70℃
Humidity	5%~80%
Altitude	Operating: below 3 000 meters
	Non-operating: below 15 000 meters
Cooling Method	Fan Cooling

Note^[1]: The accuracy parameters are acquired via calibration under 25℃ after 1-hour warm-up.

Note^[2]: The maximum time required for the output to change accordingly after receiving the **APPLY** and **SOURCE** commands.

Note^[3]: The variation of the output within 8 hours after 30-minute warm-up when the load circuit and environment temperature are constant.

DP831/DP832/DP821/DP811 Specifications

Model	Number of Channels
DP832	3
DP831	3
DP821	2
DP811	1 (two output ranges)

DC Output (0°C to 40°C)			
Channel (Range)		Voltage/Current	OVP/OCF
DP832	CH1	0 to 30V/0 to 3A	10mV to 33V/1mA to 3.3A
	CH2	0 to 30V/0 to 3A	10mV to 33V/1mA to 3.3A
	CH3	0 to 5V/0 to 3A	10mV to 5.5V/1mA to 3.3A
DP831	CH1	0 to 8V/0 to 5A	10mV to 8.8V/1mA to 5.5A
	CH2	0 to 30V/0 to 2A	10mV to 33V/1mA to 2.2A
	CH3	0 to -30V/0 to 2A	-10mV to -33V/1mA to 2.2A
DP821	CH1	0 to 60V/0 to 1A	10mV to 66V/10mA to 1.1A
	CH2	0 to 8V/0 to 10A	10mV to 8.8V/10mA to 11A
DP811	Range1	0 to 20V/0 to 10A	10mV to 22V/10mA to 11A
	Range2	0 to 40V/0 to 5A	10mV to 44V/10mA to 5.5A

Load Regulation Rate, \pm (Output Percentage + Offset)	
Voltage	$<0.01\% + 2\text{mV}$
Current	$<0.01\% + 250\mu\text{A}$

Linear Regulation Rate, \pm (Output Percentage + Offset)	
Voltage	$<0.01\% + 2\text{mV}$
Current	$<0.01\% + 250\mu\text{A}$

Ripple and Noise (20Hz to 20MHz)	
Normal Mode Voltage	DP832/DP831/DP821: $<350\mu\text{Vrms}/2\text{mVpp}$ DP811: $<350\mu\text{Vrms}/3\text{mVpp}$
Normal Mode Current	$<2\text{mArms}$

Annual Accuracy ^[1] (25°C ± 5°C), ± (Output Percentage + Offset)					
Channel		Programming		Readback	
		Voltage	Current	Voltage	Current
DP832	CH1	0.05% + 20mV	0.2% + 5mA	0.05% + 10mV	0.15% + 5mA
	CH2	0.05% + 20mV	0.2% + 5mA	0.05% + 10mV	0.15% + 5mA
	CH3	0.1% + 5mV	0.2% + 5mA	0.1% + 5mV	0.15% + 5mA
DP831	CH1	0.1% + 5mV	0.2% + 10mA	0.1% + 5mV	0.2% + 10mA
	CH2	0.05% + 20mV	0.2% + 5mA	0.05% + 10mV	0.1% + 5mA
	CH3	0.05% + 20mV	0.2% + 5mA	0.05% + 10mV	0.1% + 5mA
DP821	CH1	0.1% + 25mV	0.2% + 10mA	0.1% + 25mV	0.15% + 10mA
	CH2	0.05% + 10mV	0.2% + 10mA	0.05% + 5mV	0.15% + 10mA
DP811	CH1	0.05% + 10mV	0.1% + 10mA	0.05% + 10mV	0.1% + 10mA

Resolution								
Channel			Programming		Readback		Display	
			Voltage	Current	Voltage	Current	Voltage	Current
DP832	Standard	CH1	10mV	1mA	10mV	1mA	10mV	10mA
		CH2	10mV	1mA	10mV	1mA	10mV	10mA
		CH3	10mV	1mA	10mV	1mA	10mV	10mA
	With the high-resolution option	CH1	1mV	1mA	0.1mV	0.1mA	1mV	1mA
		CH2	1mV	1mA	0.1mV	0.1mA	1mV	1mA
		CH3	1mV	1mA	0.1mV	0.1mA	1mV	1mA
DP831	Standard	CH1	1mV	1mA	1mV	1mA	10mV	10mA
		CH2	10mV	1mA	1mV	1mA	10mV	10mA
		CH3	10mV	1mA	1mV	1mA	10mV	10mA
	With the high-resolution option	CH1	1mV	0.3mA	0.1mV	0.1mA	1mV	1mA
		CH2	1mV	0.1mA	0.1mV	0.1mA	1mV	1mA
		CH3	1mV	0.1mA	0.1mV	0.1mA	1mV	1mA
DP821	Standard	CH1	10mV	1mA	10mV	1mA	10mV	1mA
		CH2	10mV	10mA	10mV	10mA	10mV	10mA
	With the high-resolution option	CH1	1mV	0.1mA	1mV	0.1mA	1mV	0.1mA
		CH2	1mV	1mA	1mV	1mA	1mV	1mA
DP811	Standard	CH1	10mV	10mA	1mV	1mA	10mV	10mA
	With the high-resolution option	CH1	1mV	0.5mA	0.1mV	0.1mA	1mV	1mA
	With the high-resolution option	CH1	10mV	1mA	10mV	1mA	10mV	1mA

Transient Response Time

Less than 50 μ s for output voltage to recover to within 15mV following a change in output current from full load to half load or vice versa.

Command Processing Time^[2]

<118ms

OVP/OC

Accuracy, \pm (Output Percentage + Offset)

0.5% + 0.5V/0.5% + 0.5A

Voltage Programming Control Speed (1% within the total variation range)

Channel		Rise		Fall	
		Full Load	No Load	Full Load	No Load
DP832	CH1	<50ms	<33ms	<46ms	<400ms
	CH2	<50ms	<38ms	<46ms	<400ms
	CH3	<15ms	<14ms	<24ms	<100ms
DP831	CH1	<18ms	<17ms	<20ms	<200ms
	CH2	<33ms	<36ms	<44ms	<400ms
	CH3	<35ms	<42ms	<45ms	<400ms
DP821	CH1	<110ms	<30ms	<110ms	<800ms
	CH2	<15ms	<15ms	<20ms	<400ms
DP811	CH1	<45ms	<42ms	<51ms	<1089ms

Temperature Coefficient per $^{\circ}\text{C}$, \pm (Output Percentage + Offset)

Channel		Voltage	Current
DP832	CH1	0.01% + 5mV	0.01% + 2mA
	CH2	0.01% + 5mV	0.01% + 2mA
	CH3	0.01% + 2mV	0.01% + 2mA
DP831	CH1	0.01% + 2mV	0.02% + 3mA
	CH2	0.01% + 2mV	0.02% + 3mA
	CH3	0.01% + 2mV	0.02% + 3mA
DP821	CH1	0.01% + 3mV	0.02% + 3mA
	CH2	0.01% + 3mV	0.02% + 3mA
DP811	CH1	0.01% + 3mV	0.02% + 3mA

Stability ^[3] , ± (Output Percentage + Offset)			
Channel		Voltage	Current
DP832	CH1	0.02% + 2mV	0.05% + 2mA
	CH2	0.02% + 2mV	0.05% + 2mA
	CH3	0.01% + 1mV	0.05% + 2mA
DP831	CH1	0.03% + 1mV	0.1% + 3mA
	CH2	0.02% + 2mV	0.05% + 1mA
	CH3	0.02% + 2mV	0.05% + 1mA
DP821	CH1	0.02% + 1mV	0.1% + 1mA
	CH2	0.02% + 1mV	0.1% + 1mA
DP811	CH1	0.02% + 1mV	0.1% + 1mA

Mechanical	
Dimensions	239mm (W) x 157mm (H) x 418mm (D)
Weight	DP832: 10.5kg DP831: 9.75kg DP821: 10.0kg DP811: 10.3kg

Power	
AC Input (50Hz-60Hz)	100Vac ± 10%, 115Vac ± 10%, 230Vac ± 10% (maximum 250Vac)
Maximum Input Power	DP832: 521VA DP831: 416VA DP821: 450VA DP811: 503VA

I/O	
USB DEVICE	1
USB HOST	1
LAN	1 (optional)
RS232	1 (optional)
Digital IO	1 (optional)
USB-GPIB	1 (optional, extend a GPIB interface using the USB-GPIB interface converter option)
Rear Panel Output Interface	1 for DP811

Environment	
Cooling Method	Fan Cooling
Working Temperature	0°C to 40°C
Storage Temperature	-40°C to 70°C
Humidity	5% to 80% relative humidity
Altitude	Below 1 500m
IP Degree	IP20
Pollution Degree	PD2
Over Voltage Category	OVC II
Operation Location	Indoor use only; not for wet condition

Note^[1]: The accuracy parameters are acquired via calibration under 25°C after 1-hour warm-up.

Note^[2]: The maximum time required for the output to change accordingly after receiving the APPLy and SOURce commands.

Note^[3]: The variation of the output within 8 hours after 30-minute warm-up when the load circuit and environment temperature are constant.